



THE UNIVERSITY *of* EDINBURGH

Edinburgh Research Explorer

Preliminary results of CoQtz-N: A quartz reference material for terrestrial in-situ cosmogenic ^{10}Be and ^{26}Al measurements

Citation for published version:

Binnie, SA, Dewald, A, Heinze, S, Voronina, E, Hein, A, Wittmann, H, Von Blanckenburg, F, Hetzel, R, Christl, M, Schaller, M, Léanni, L, Aster Team, Hippe, K, Vockenhuber, C, Ivy-ochs, S, Maden, C, Fülöp, R, Fink, D, Wilcken, KM, Fujioka, T, Fabel, D, Freeman, SPHT, Xu, S, Fifield, LK, Akçar, N, Spiegel, C & Dunai, TJ 2019, 'Preliminary results of CoQtz-N: A quartz reference material for terrestrial in-situ cosmogenic ^{10}Be and ^{26}Al measurements', *Nuclear Instruments and Methods in Physics Research Section B: Beam Interactions with Materials and Atoms*. <https://doi.org/10.1016/j.nimb.2019.04.073>

Digital Object Identifier (DOI):

[10.1016/j.nimb.2019.04.073](https://doi.org/10.1016/j.nimb.2019.04.073)

Link:

[Link to publication record in Edinburgh Research Explorer](#)

Document Version:

Peer reviewed version

Published In:

Nuclear Instruments and Methods in Physics Research Section B: Beam Interactions with Materials and Atoms

General rights

Copyright for the publications made accessible via the Edinburgh Research Explorer is retained by the author(s) and / or other copyright owners and it is a condition of accessing these publications that users recognise and abide by the legal requirements associated with these rights.

Take down policy

The University of Edinburgh has made every reasonable effort to ensure that Edinburgh Research Explorer content complies with UK legislation. If you believe that the public display of this file breaches copyright please contact openaccess@ed.ac.uk providing details, and we will remove access to the work immediately and investigate your claim.



Preliminary results of CoQtz-N: A quartz reference material for terrestrial in-situ cosmogenic ^{10}Be and ^{26}Al measurements

S. A. Binnie^{a,1}; T. J. Dunai^a; A. Dewald^b; S. Heinze^b; E. Voronina^a; A. Hein^c; H. Wittmann^d; F. von Blanckenburg^d; R. Hetzel^e; M. Christl^f; M. Schaller^g; L. Léanni^h; ASTER Team^{h,2}; K. Hippe^f; C. Vockenhuber^f; S. Ivy-Ochs^f; C. Madenⁱ; R.-H. Fülöp^{j,k}; D. Fink^k; K. M. Wilcken^k; T. Fujioka^k; D. Fabel^l; S.P.H.T. Freeman^l; S. Xu^l; L. K. Fifield^m; N. Akçarⁿ; C. Spiegel^o.

^a Institute of Geology and Mineralogy, University of Cologne, Zùlpicher Str. 49b, 50674 Cologne, Germany

^b Institut für Kernphysik, University of Cologne, 50937 Cologne, Germany

^c School of GeoSciences, University of Edinburgh, Drummond St, Edinburgh, EH8 9XP, UK

^d Helmholtz Centre Potsdam, GFZ German Research Centre for Geosciences, Telegrafenberg, 14473 Potsdam, Germany

^e Institut für Geologie und Paläontologie, Westfälische Wilhelms-Universität Münster, Corrensstraße 24, D-48149 Münster, Germany

^f Laboratory of Ion Beam Physics, ETH Zurich, CH-8093 Zurich, Switzerland

^g University of Tuebingen, Department of Geosciences, Wilhelmstrasse 56, 72074 Tuebingen, Germany

^h Aix-Marseille Univ., CNRS, IRD, Coll. France, UM 34 CEREGE, Technopôle de l'Environnement Arbois-Méditerranée, BP80, 13545 Aix-en-Provence, France

ⁱ Institute of Geochemistry and Petrology, ETH Zurich, CH-8092 Zurich, Switzerland

^j School of Earth and Environmental Sciences, University of Wollongong, NSW 2522 Australia

^k Australian Nuclear Science and Technology Organisation (ANSTO), Lucas Heights, NSW 2234 Australia

^l Scottish Universities Environmental Research Centre (SUERC), East Kilbride G75 0QF, UK

^m Department of Nuclear Physics, Research School of Physical Sciences and Engineering, The Australian National University, ACT 0200, Australia

ⁿ University of Bern, Institute of Geological Sciences, Baltzerstrasse 1-3, Bern, Switzerland

^o Universität Bremen, FB5 – Geowissenschaften, Postfach 330 440, 28344 Bremen, Germany

¹ corresponding author

² G. Aumaître; D. L. Bourlès; K. Keddadouche

Abstract

There is growing interest in geochronological applications of terrestrial *in situ*-produced cosmogenic nuclides, with the most commonly measured being ^{10}Be and ^{26}Al in quartz. To extract and then separate these radionuclides from quartz and prepare them in the oxide form suitable for accelerator mass spectrometry (AMS) requires extensive and careful laboratory processing. Here we discuss the suitability of a crushed, sieved and etched, sub-aerially exposed vein quartz specimen (CoQtz-N) to act as a reference material for chemical laboratory preparation and AMS measurements. Splits of CoQtz-N were distributed to eleven target preparation laboratories. The CoQtz-N ^{10}Be targets were then measured at seven different AMS facilities and five of the preparation laboratories had their ^{26}Al targets measured at four different AMS facilities. We show that CoQtz-N splits are sufficiently homogeneous with regard to nuclide concentrations, that it has been cleaned of any atmospheric derived (i.e. meteoric) ^{10}Be and that it has low concentrations of the major elements that can interfere with Be and Al extraction chemistry and AMS measurements. ~~Average ^{10}Be results from some laboratories differ by statistically significant amounts and we briefly discuss possible reasons for the discrepancies. The data which passes our outlier criteria tests is used to~~ We derive preliminary concentrations for ^{10}Be and ^{26}Al in CoQtz-N as $2.54\text{--}53 \pm 0.02\text{--}09 \times 10^6$ at/g and $15.7\text{--}6 \pm 0.1\text{--}4\text{--}6 \times 10^6$ at/g, respectively, at the ~~estimated~~ 95% confidence limit.

Keywords: ^{26}Al ; ^{10}Be ; CoQtz-N; Cosmogenic nuclides; ~~Intercomparison~~; Reference material.

1. Introduction

Over the last few decades there has been a growing interest in measuring cosmic ray-produced ^{10}Be and ^{26}Al within quartz to determine rates of geomorphological processes, surface exposure ages or burial histories (Granger et al., 2013). The trace amounts of ^{10}Be and ^{26}Al produced in quartz require sensitive measurements by accelerator mass spectrometry (AMS) and the preparation of geological samples into a suitable form for such analysis requires careful processing in the laboratory. Several different approaches for preparing ^{10}Be and ^{26}Al AMS targets from cleaned quartz separates are used by different laboratories (e.g. Binnie et al., 2015; Child et al., 2000; Corbett et al., 2016; Kohl and Nishiizumi, 1992; von Blanckenburg et al., 2004), while AMS measurements are calibrated against various standard reference materials and performed using different accelerator configurations and analysis schemes (Merchel et al., 2012). There is, therefore, a need to be able to compare the ^{10}Be and ^{26}Al concentrations (i.e. atoms/gram sample) being reported by different groups with respect to their chemistry processing techniques and their analytical performance.

The standard method of analyzing how well results from different laboratories agree is by inter-laboratory comparison, or proficiency testing. Such trials allow laboratories to examine their performance and make corrections where needed (Scott et al., 2007). However, this requires available common materials, ideally of known, or at least agreed-upon (i.e. nominal), values. Inter-laboratory comparisons were carried out as part of the Cronus-Earth and Cronus-EU projects (Phillips et al., 2016) using rock samples prepared from appropriate lithologies. This work investigated the suitability of specific materials for cosmogenic ^{21}Ne (Vermeesch et al., 2015), ^3He (Blard et al., 2015), ^{10}Be and ^{26}Al measurements (Jull et al., 2015). One bedrock and one beach sand specimen, termed CRONUS-A and CRONUS-N, respectively, were collected and measured by several groups participating in the Cronus projects for the purpose of comparing ^{10}Be and ^{26}Al . However, concerns have been raised regarding the

homogeneity of CRONUS-N (Bierman et al., 2017), while the consensus ^{10}Be concentration value derived for CRONUS-A is very high, at 3.303×10^7 at/g (Jull et al., 2015). ~~Therefore, Thus, t~~there is still the need for a quartz reference materials, with lower concentrations more typical of the majority of ^{10}Be and ^{26}Al measurements, that which can be considered in some sense 'typical' of cosmogenic ^{10}Be and ^{26}Al sample preparation and measurement prepared and measured alongside samples. In addition, the Cronus results highlight a need for further comparison studies of ^{10}Be and ^{26}Al the need for further work in this area (Jull et al., 2015). Having a full procedural reference material that is pre-etched quartz as opposed to a calibration reference material in the form of Be oxide, for example (Merchel et al., 2012), allow comparisons to be made not only of the AMS but also the results from the sample preparation laboratories. However, this introduces the added complexity of determining whether scatter, or any bias observed, derives from preparation of samples as targets in the laboratory or during the AMS measurement.

In this contribution we present details of the preparation and the initial measurements of CoQtz-N, a quartz material that we recommend should be used as an in-house, chemistry procedure reference material by the AMS community, in proficiency and full reproducibility testing, as well as for collaborative inter-laboratory investigations. We discuss the intra- and inter-laboratory results and present preliminary consensus values for the concentrations of ^{10}Be and ^{26}Al . Finally, we briefly discuss potential reasons for the differences observed in results from different groups and consider what remains to be investigated to mitigate these differences.

2. CoQtz-N production, material tests and concentration determinations

2.1. CoQtz-N production and distribution

Formatted: Superscript

Formatted: Superscript

Formatted: Superscript

Formatted: Superscript

The CoQtz-N quartz material was produced from a single boulder of vein quartz that was part of a lag deposit mantling a low relief surface near Hakos in Namibia (Figure 1). The sample was broken-up at the University of Cologne with a sledgehammer and fragments were visually inspected for any impurities; a few fragments that contained black tourmaline were discarded. The quartz was then crushed with a jaw crusher and disc mill and dry sieved to obtain the 250 – 710 μm size fraction. This portion was sent to the University of Edinburgh where it was etched three times in an ultrasonic bath using a 2% HF / 2% HNO_3 acid solution with a ratio of 1 g of quartz per 20 ml of dilute acid mixture. The final etch used analytical grade acids diluted in 18 M Ω -cm deionized water. The total quartz mass lost due to this etching was ~15%. Around 25 kg of etched quartz was returned to the University of Cologne where it was homogenized and then split using an 8-way rotating cone splitter fed by a vibratory chute. Splits of ~165 g were packaged in screw-top plastic beakers, labeled and distributed [between 2014 and 2016](#) to 11 cosmogenic nuclide sample preparation laboratories, herein termed 'laboratories' for brevity (Table 1). CoQtz-N recipients were instructed not to clean the quartz any further but to dissolve it directly from the container. Five grams was suggested to be an appropriate, though not obligatory amount to dissolve in order to mimic routine samples but not exhaust the supply of CoQtz-N too rapidly.

2.2. Material tests

The purity of CoQtz-N was determined by ICP-OES (inductively coupled plasma - optical emission spectrometry) measurements at the University of Cologne. In brief, five 1 g portions were dissolved in concentrated trace-metal grade HF/ HNO_3 , heated to dryness three times in the presence of aqua regia before each sample was prepared as four dilutions for standard addition in 0.3M HNO_3 . One reagent blank was prepared the same way in parallel with the samples. Measurements were performed on a Spectro Arcos ICP-OES using an axial configuration.

Subsequent to receiving some initial results, it was found that one laboratory had acid etched a portion of their CoQtz-N samples prior to dissolution. To test that additional etching would not influence the nuclide concentrations, a batch of six CoQtz-N splits were prepared at the University of Cologne, where two of the splits were dissolved directly from the container, i.e. no further etching, two of the splits were etched once and two splits were rinsed and etched a second time. Etching in these cases was overnight in an ultrasonic bath, using a 1% HF / 1% HNO₃ acid solution with a ratio of 1 g of quartz per 100 ml of dilute acid mixture. Specified grade acids and 18 MΩ-cm water were used. There was an approximate 20% loss of quartz mass from the splits that were etched twice.

2.3. Concentration determinations

Eleven laboratories reported CoQtz-N measurements of ¹⁰Be undertaken on seven different AMS facilities and five of those laboratories also prepared and measured ²⁶Al targets that were measured on four of the seven different AMS facilities (Table 1). Herein, these AMS facilities are labelled as AMS 1 through AMS 7. Reporting from each recipient was done via a standardized Microsoft Excel® spreadsheet that asked for the following information: the ¹⁰Be/⁹Be, or ²⁶Al/²⁷Al, ratio for each CoQtz-N sample and relevant reagent blank; the mass of ⁹Be in the carrier added to each CoQtz-N sample and relevant reagent blank; the name/brand and concentration of Be and Al carriers used, plus the final mass of ²⁷Al in the samples and blanks and the method of this determination. For each measurement reported, calculations following Eq. 1a and Eq. 1b for the concentration of ¹⁰Be (*N_{Be}*) and ²⁶Al (*N_{Al}*) in atoms per gram were performed by the spreadsheet.

$$N_{Be} = \frac{\left[\frac{{}^{10}Be}{{}^9Be}_Q \cdot c_{BeQ} \cdot L \cdot \frac{1}{u_{Be}} \right] - \left[\frac{{}^{10}Be}{{}^9Be}_B \cdot c_{BeB} \cdot L \cdot \frac{1}{u_{Be}} \right]}{m}$$

Eq. 1a

$$N_{Al} = \frac{\left[\frac{{}^{26}Al}{{}^{27}Al}_Q \cdot c_{AlT} \cdot L \cdot \frac{1}{u_{Al}} \right] - \left[\frac{{}^{26}Al}{{}^{27}Al}_B \cdot c_{AlB} \cdot L \cdot \frac{1}{u_{Al}} \right]}{m}$$

Eq. 1b

In equations [1a] and [1b], subscripts *Q* and *B* on the ${}^{10}\text{Be}/{}^9\text{Be}$, or ${}^{26}\text{Al}/{}^{27}\text{Al}$, ratios are the CoQtz-N sample and reagent blank AMS measurements, respectively. The mass of ${}^9\text{Be}$ carrier used in the sample and blank are given by c_{BeQ} or c_{BeB} , respectively. The total ${}^{27}\text{Al}$ mass in the sample is given by c_{AlT} and in the blank by c_{AlB} . Note, c_{AlT} refers to the ${}^{27}\text{Al}$ within the quartz plus any ${}^{27}\text{Al}$ added as carrier. L is Avogadro's constant, u_B and u_{Al} are the respective atomic masses of ${}^9\text{Be}$ and ${}^{27}\text{Al}$. The mass of CoQtz-N dissolved is denoted by m . Laboratories were asked to give final AMS analytical measurement uncertainties and the stable isotope mass uncertainties as one standard deviation. The uncertainties in the concentrations of ${}^{10}\text{Be}$ and ${}^{26}\text{Al}$ were also calculated by the spreadsheet, using standard error propagation formula (Bevington and Robinson, 2003). Additionally, CoQtz-N recipients were asked: what metal matrix was mixed with the BeO and Al_2O_3 before samples were pressed into targets and if this matched that in the AMS standard reference material (SRM) used for calibration; which AMS SRMs were used for the measurement; what nominal values were used for the AMS SRMs and in the case of ${}^{10}\text{Be}/{}^9\text{Be}$ standards, what value was assumed for the half-life of ${}^{10}\text{Be}$.

3. Results [and statistical analysis](#)

3.1. Material purity

ICP-OES measurements of the concentrations of the major elements of most interest in CoQtz-N are given in Table 2. The concentration of Al is relatively low at 18.4 ± 0.6 ppm. Ti is sometimes cited as problematic for causing reduced Be chemistry yields and lower AMS ${}^9\text{Be}$ negative ion-source beam

currents (e.g. Hunt et al 2008), but the Ti concentration is also relatively low at 7.6 ± 2.6 ppm. No differences in ^{10}Be concentrations were observed due to further etching of the CoQtz-N, as can be seen by comparing the results of the etched and non-etched concentrations (Figure 2), so we do not exclude any results where additional HF etching was performed.

3.2. Initial measurements and corrections

Figure 3a shows the results from laboratories 1, 2, 3, 4 and 7 for the 63 BeO targets that were all measured on AMS 1, plotted against their [average](#) analyzed ^9Be current as a fraction of the average ^9Be current of the [primary](#) standards used in that run (relative ^9Be current). A significant positive correlation is observed with respect to ^{10}Be concentration versus relative ^9Be current, as well as a degree of clustering per laboratory. This explains an initially observed significant difference in the average ^{10}Be concentrations between laboratories 1, 2, 3 and 4 measured on AMS 1. Consequently, the ^{10}Be concentrations that were measured on AMS 1 were re-normalized to the average current of the standards used in the same run (Figure 3b). This produces an increase in the average ^{10}Be concentrations of laboratories 1, 2 and 4 of 0.8%, 5.1% and 5.3%, respectively, and means that the average ^{10}Be concentrations of each of the four laboratories overlap within 1 standard deviation. The average concentration of laboratory 3 does not change. The single result from laboratory 7, also measured on AMS 1, increases by 2.1%. All results reported for these laboratories include this adjustment, for which no additional analytical uncertainties have been included.

To date, 89 ^{10}Be measurements and 23 ^{26}Al measurements have been reported. ^{10}Be and ^{26}Al concentrations ~~from all the seven AMS facilities~~ are given in Figures 4 and 5, respectively, where each plot shows the results for a single laboratory (the accelerators are given different symbols, laboratories are given different colors). All laboratories had their samples measured on a single AMS facility except

laboratories 3 and 10 who measured ^{10}Be at two different accelerators. Blank subtractions reduced ^{10}Be concentrations by between 0.1 to 4.5 %, though the majority of corrections were less than 1% (Figure 6). The larger blank subtractions are typically associated with smaller sample masses (e.g., <1 g instead of 5 g), rather than higher reagent blank $^{10}\text{Be}/^9\text{Be}$ measurements. All reagent blank subtractions for Al were less than 0.5%. [Most laboratories reported blanks that were prepared in the same batch as the CoQtz-N samples, while one laboratory used a long-term average blank value for both \$^{26}\text{Al}\$ and \$^{10}\text{Be}\$.](#) We note that AMS $^{10}\text{Be}/^9\text{Be}$ measurements were normalized to either: the NIST ^{10}Be SRM 4325 assuming the nominal $^{10}\text{Be}/^9\text{Be}$ value of 2.79×10^{-11} (Nishiizumi et al., 2007); the ICN standard dilution series using the values reported in Nishiizumi et al. (2007); or they were calibrated against in-house standards that were traceable to these values. All $^{26}\text{Al}/^{27}\text{Al}$ AMS measurements were normalized to the standards of Nishiizumi (2004), or to in-house standards, cross-calibrated against the consensus values reported in the round-robin exercise of Merchel and Bremser (2004). Be and Al oxides prepared from CoQtz-N were mixed with either Nb (Be) or Ag (Be and Al) and all [of the laboratories-AMS facilities measured samples usingused](#) standards pressed with the same metal [as the CoQtz-N samples](#).

Formatted: Superscript

Formatted: Superscript

3.3. Summary statistics for ^{10}Be and ^{26}Al concentrations

[We have derived summary statistics for the CoQtz-N results grouped by the laboratory where the samples were prepared. The results reported for each laboratory are not independent of the AMS facility where the measurements were made and this point will be discussed again briefly in section 3.4.](#) For laboratories [where more than one result was that](#) obtained [more than one result](#), the arithmetic and error weighted means plus associated uncertainties are shown in Tables 3 and 4. The median may provide a more robust estimate of central tendency when [few measurements have been made sample sizes are small](#) (Dean and Dixon, 1950) and this, plus the 25th and 75th percentiles, are given for laboratories with five results or more. Figures 7a and 7b compare the arithmetic mean and 95%

confidence intervals, plus medians where appropriate, for all laboratories with two or more ^{10}Be or ^{26}Al results. The error weighted mean concentrations and the estimated standard error of the weighted mean for each laboratory are also provided in Tables 3 and 4 but are not discussed further here. The reduced Chi-square, or mean square weighted deviation (MSWD) values are determined for ^{10}Be measurements from laboratories 1, 2, 3, 6 and 11 (Table 3) and for ^{26}Al measurements from laboratory 1 and 11 (Table 4). MSWD values on the order of 1 may be interpreted to mean that the uncertainties reported for individual measurements from a particular laboratory approximately agree with the scatter observed when a number of replicate measurements are made. In this way, it can be used as an indicator of whether or not laboratories [and/or the AMS facilities where the measurements were made](#), are adequately characterizing their analytical uncertainties. However, the uncertainty in the MSWD value is large when there are few degrees of freedom, that is, when sample populations are small (Wendt and Carl, 1991). Therefore, we do not derive the MSWD when there are less than seven results reported from a given laboratory. The MSWD results are discussed further in section 4.2.

Potential outliers were considered for each individual laboratory. Laboratory 1 has a single, high ^{10}Be measurement that both Grubbs and Dixon methods (Taylor, 1987) identify as an outlier ($P < 0.01$). This result is identified in Figure 4. However, based on the analytical uncertainties of the individual measurements it is not an unexpected result, as the measurement lies less than three of its standard deviations from the mean laboratory value, where $n=21$. As neither of the above methods of outlier identification take into account uncertainties and as nothing unusual was observed during the preparation or measurement of this sample that would explain the high value, we do not omit this result. However, we note that it is one of thirteen measurements that are rejected during the second stage of deriving a [consensus value](#) [filtered error weighted mean](#) (see Section 3.4). Neither Grubbs nor Dixon methods identify any outliers in the [laboratories that measured \$^{26}\text{Al}\$ results reported](#).

Formatted: Highlight

3.4. ^{10}Be concentration characterization

We compare ~~two~~[three](#) different approaches of characterizing the nuclide concentrations of CoQtz-N. The first is the approach of Ku (1969), termed the ‘grand average’ by Taylor (1987), who suggests its application to pool laboratory averages where different numbers of measurements have been reported and different amounts of dispersion exist. The result is in essence a weighted mean of the laboratory averages, where the weights are inversely proportional to the variances of the mean from each laboratory. This allows laboratories that make more measurements, or that have more tightly clustered datasets to be given more emphasis in the final result. The variance of the grand average is then the reciprocal of the sum of the weights.

The second approach is described by Rozanski et al. (1992) and was used for combining the ^{14}C data from many laboratories during [early](#) inter-laboratory comparison exercises (Scott et al., 2003). It is the approach used by Jull et al. (2015) to provide preliminary ^{10}Be concentration values for the Cronus-Earth reference materials. This approach, [herein termed the ‘filtered EWM’ \(filtered error weighted mean\)](#), considers all the results as a single dataset, rather than taking laboratory averages, and uses two stages of measurement elimination. The first stage rejects measurements more than three multiples of the interquartile range from the median and then calculates a new median. The second stage considers whether individual results that passed stage one deviate from the new median by more than two multiples of their measurement uncertainty, rejecting those that do. The remaining results are used to derive an [average](#) ~~‘consensus-value’~~ by taking an error weighted mean. This approach aims to remove potential outliers and results whose quoted errors may be underestimated. Additionally, Rozanski et al. (1992) suggest that the Chi-square test proposed by Ward and Wilson (1978) is used to determine

whether the remaining results come from a single population, incorporating an additional multiplier to the estimate of the standard error when the null hypothesis is rejected.

The third method we use to characterize the radionuclide concentrations of CoQtz-N is ‘linear mixed modelling’ and our approach is similar to that of the most recent ¹⁴C inter-laboratory comparison exercise (Scott et al. 2017). Mixed (random effect) models allow variance to be partitioned into multiple components, in this case the laboratory and the AMS facility. Unlike the above two methods, it accommodates the interdependency of results that have been prepared in different laboratories but measured using the same AMS facility. For example, it caters for laboratories 1, 2, 3, 4 and 7 all having measured ¹⁰Be using AMS 1 and thus having a mutual source of variance. Our model takes the form shown in equation 2:

$$Y_{ijk} = \mu + \alpha_i + \beta_{ij} + \varepsilon_{ijk}$$

where Y is the radionuclide concentration measured in the kth sample reported from the jth laboratory and measured at the ith AMS facility. We note that: k = 1,...,K, where K is the number of replicate CoQtz-N measurements from a given laboratory; j = 1,...,J, where J is the number of laboratories; and that i = 1,...,I, where I is the number of AMS facilities. μ is the overall mean value, α is the random effect for an AMS facility, β is the random effect for a preparation laboratory and ε is the deviation from the overall mean not accounted for by the previous two effects.

We employ a hierarchical design that nests laboratories ‘within’ AMS facilities, as many laboratories may measure at a single AMS facility but the reverse is less common. In the two cases where a single laboratory has measured ¹⁰Be in CoQtz-N samples at two different AMS facilities we have treated the

Formatted: Superscript

Eg. 2

Formatted: Not Superscript/ Subscript, Highlight

Formatted: Highlight

Formatted: Right

Formatted: Font: Symbol

Formatted: Not Highlight

Formatted: Font: Symbol

Formatted: Not Highlight

Formatted: Font: Symbol

Formatted: Not Highlight

Formatted: Not Highlight

Formatted: Font: Symbol

Formatted: Not Highlight

Formatted: Not Highlight

Formatted: Not Highlight

Formatted: Superscript

[results as belonging to two separate groups. For example, for the purposes of the modelling, the results of laboratory 3 are separated and nested within either AMS 1 or AMS 2 \(see figure 4\).](#)

An estimate of the mean radionuclide concentration and corresponding variance is required from each laboratory in order to calculate a grand average. We include laboratories that have reported three or more measurements (Table 3), so as to get a reasonable estimate of variance, and obtain a result of $2.53 \pm 0.02 \times 10^6$ atoms $^{10}\text{Be/g}$ (estimated 95% Confidence Interval). The [filtered EWM](#) consensus value calculated according to Rosanski et al. (1992) produces $2.54 \pm 0.02 \times 10^6$ atoms $^{10}\text{Be/g}$ (estimated 95% Confidence Interval). During derivation of [filtered EWM](#) the consensus value no measurements were rejected in stage 1. Thirteen of the eighty-nine measurements were rejected during stage 2 (Figure 8). We fail to reject the null hypothesis that the remaining dataset is homogeneous at the 5% level and so do not add a multiplier to the estimate of the standard error of the [filtered EWM](#) consensus value. The [linear mixed modeling utilizes all the data and estimates a mean value of \$2.53 \pm 0.09 \times 10^6\$ atoms \$^{10}\text{Be/g}\$ \(95% Confidence Interval\). The above results are summarized in Table 5.](#)

Formatted: Highlight

Formatted: Highlight

Formatted: Highlight

Formatted: Superscript

Formatted: Superscript

3.5. ^{26}Al concentration characterization

Fewer measurements of ^{26}Al are reported than are of ^{10}Be . Nevertheless, we derive a grand average and consensus value as per ^{10}Be . For the grand average we calculate a value of $15.2 \pm 0.1 \times 10^6$ atoms $^{26}\text{Al/g}$ (estimated 95% Confidence Interval). The result is clearly dominated by laboratory 6, whose three measurements are very tightly clustered and thus strongly biasing the error weighted result. The [filtered EWM](#) consensus value calculated according to Rosanski et al. (1992) gives $15.7 \pm 0.4 \times 10^6$ atoms $^{26}\text{Al/g}$ (estimated 95% Confidence Interval). During derivation of the [filtered EWM](#) consensus value, no measurements were rejected in stage 1 and four of twenty-three values were rejected in stage 2 (Figure 9). There is no evidence to reject the null hypothesis that the dataset is homogeneous at the 5% level

Formatted: Highlight

Formatted: Highlight

and so no error multiplier is included in the estimate of the standard error of the weighted mean. [The result of our linear mixed modeling is a mean value of \$15.6 \pm 1.6 \times 10^6\$ atoms \$^{26}\text{Al}/\text{g}\$ \(95% Confidence Interval\). The above results are summarized in Table 5.](#)

Formatted: Superscript

Formatted: Superscript

4. Discussion

4.1 Material purity

There is no difference observed in ^{10}Be concentrations of CoQtz-N after additional HF/HNO₃ etches (Figure 2). This suggests that the cleaning of the CoQtz-N material, performed prior to splitting, was sufficient to remove any adsorbed meteoric ^{10}Be . Further cleaning of CoQtz-N is unnecessary and to reduce potential sources of contamination it should not be further processed, chemically or otherwise, prior to dissolution.

The low scatter of the five ICP-OES Al concentration measurements suggest the Al concentration within CoQtz-N splits is uniform (Table 2). Na, K, Ti and Fe show greater variability and this scatter appears largely due to one of the five 1 g portions having higher concentrations of these particular elements. This might reflect the presence of minor amounts of non-quartz minerals (e.g., rutile in the case of Ti). In any case, the concentrations of these elements are also low.

4.2 Intra-laboratory results of CoQtz-N measurements

The MSWD of the ^{10}Be results from laboratories 1 and 3 are somewhat lower than unity, at 0.49 and 0.52 respectively. The probability of obtaining an MSWD result equal to or lower than that of laboratory 1 is ~3%, meaning there is a reasonably strong likelihood that this laboratory overestimates the size of its measurement uncertainties. The MSWD result from laboratory 3 is similar to laboratory 1 but because of fewer results (i.e. fewer degrees of freedom) it is less statistically significant, with a ~16%

probability of obtaining an equal or lower MSWD value. This means it is premature to consider whether laboratory 3 is also overestimating uncertainties. The ^{10}Be concentrations from laboratory 6 result in an MSWD value of 3.46 and the probability of such a result occurring by chance is <1%. This strongly suggests that laboratory 6 is underestimating analytical uncertainties. As the majority of laboratories do not show excess scatter (Table 3), the individual splits of CoQtz-N seem to be internally homogeneous with regard to the ^{10}Be concentration, at least within typical measuring precisions of a few percent. Thus, bias should not be introduced during the sub-sampling of the splits and the material can be spooned directly from the beakers without the need for additional splitting methods. The MSWD value for ^{26}Al measurements from laboratory 1 is close to unity but the result from laboratory 11 is high at 2.32, with a probability of obtaining such a result, or higher, being ~3%. These laboratories MSWD values are constrained by a relatively small number of results (Table 4), thus, we suggest that there is within-split homogeneity also for ^{26}Al but we note that this assertion is tentative pending more data.

Laboratories 3 and 10 measured ^{10}Be on 2 different AMS (Figure 4). Laboratory 3 measurements from AMS 1 (n=4) and AMS 2 (n=5) show good agreement, suggesting these accelerators produce comparable results. The small number of measurements from laboratory 10 makes it premature to compare results. More comparisons between single laboratories and multiple accelerators are required.

4.3 Inter-laboratory results of CoQtz-N measurements

The stable ion currents of $^{10}\text{Be}/^9\text{Be}$ measurements, relative to the output of the standards, are seen as a general indicator of the quality or performance of the target. The large number of CoQtz-N $^{10}\text{Be}/^9\text{Be}$ measurements made by AMS 1 from targets prepared by five different laboratories shows that ^{10}Be concentrations may vary in relation to target performance as seen in Figure 3. It is not clear that this co-dependency is entirely attributable to the specific configuration of AMS 1 (i.e. tuning, transmission, ion

source behavior, etc.) but normalizing the data to correct for this effect resolves what would otherwise be a discrepancy between average CoQtz-N ^{10}Be concentrations. The chemistries employed by laboratories 1 through 4 and laboratory 7 for target preparation are different and will likely have a fundamental control over the typical relative stable ion currents. Several other factors could also contribute to the average laboratory target performance, including: 1. the experience and skill of those preparing the targets; 2. the typical research applications of the research group, which can dictate the purity of the starting material, i.e. fluvial or colluvial sediments can be relatively rich in resistant mineral impurities, making it more challenging to obtain pure quartz and subsequently to separate Be from other elements during sample processing (Binnie et al., 2015; Corbett et al., 2016; Mifsud et al., 2013); 3. the type of metal matrix used during target pressing, the ratio of metal to BeO and the homogeneity of the mixing between the metal and the oxide are important considerations (Hunt et al. 2006; Merchel et al., 2008; Stone et al., 2004). The range of ^9Be currents that were obtained by AMS 1 during the measurements of CoQtz-N from multiple laboratories allows the recognition of a relationship with ^{10}Be concentrations and current that might not be apparent if the target measurements had performed within a narrower range of currents, as is often the case for measurements of an in-house standard from individual target preparation laboratories. More generally, findings such as this illustrate the advantage of different laboratories and accelerators making many measurements of quartz reference materials, such as CoQtz-N, over the long-term.

The usefulness of CoQtz-N to the user community depends in part on an appropriate characterization of the nuclide concentrations it contains. Here we considered ~~two-three~~ approaches for this determination, termed ~~the the~~ grand average ~~and, the the~~ filtered EWM ~~consensus value~~ and linear mixed modelling.

The near identical ^{10}Be concentrations derived by the different methods may be coincidental but provide some confidence in the result. For the grand average ^{10}Be concentration we included

Formatted: Highlight

laboratories with three or more measurements, but including only the three laboratories with the most measurements (laboratories 1, 2 and 11, $n \geq 10$) would increase the average by only 0.4%. This is because weighting by the inverse of the variance of the mean (n/σ^2) has the consequence that the grand average is strongly influenced by those laboratories that have reported the most measurements. In contrast, the difference found between the averaging methods when it comes to ^{26}Al concentrations is due to the very low spread (i.e. excellent reproducibility) of the three values from laboratory 6 and the tendency of the grand average to place more weighting on mean values with low dispersion. Thus, in the case of ^{26}Al there is a strong bias towards the mean of laboratory 6 that does not occur in the [filtered EWM consensus value](#) or [linear mixed modelling](#) approaches, which treats every measurement [independently/separately](#). In general, ^{26}Al concentration measurements tend to have higher analytical uncertainties and to show more inter-laboratory scatter than ^{10}Be (Jull et al., 2015; Phillips et al., 2016) and so our characterization of the ^{26}Al concentration of CoQtz-N would benefit from more measurements. [There is little difference between the average values estimated using the filtered EWM and linear mixed modelling approaches, but linear mixed modelling recognizes there are common sources of variation and provides appropriately adjusted uncertainties. Accordingly, we](#) ~~For now we favor the results of the consensus value~~ [linear mixed modelling result as a preliminary concentrations value for both \$^{10}\text{Be}\$ and \$^{26}\text{Al}\$ concentration.](#)

Formatted: Highlight

By standardizing methods of concentration calculation we aimed to exclude blank subtraction as an additional source of dispersion between [laboratories the CoQtz-N results](#). Other causes for the differences observed could include inappropriate characterization of ^9Be carrier concentrations (Merchel et al., 2013), or incorrect determination of the ^{27}Al in the sample (Fujioka et al., 2015). Precise and accurate determination of ^{27}Al is as critical as the quality of the ^{26}Al AMS measurement. In addition, improper calibration of laboratory balances, or non-trivial effects of static during weighing, can be problematic, as can systematic bias introduced by individuals preparing the targets. Indeed, this last

effect in particular is difficult to investigate unless there is already a long-term record of laboratory in-house standards. In addition, as discussed above, comprehensive examinations of target performance effects are needed. It is not yet possible to resolve whether the differences we observe between ~~laboratory~~ averages [calculated at the level of individual laboratories](#) are introduced during the processing or during the AMS measurements. Though the differences between the average ^{10}Be concentrations from various groups are small, they are more apparent in the few ^{26}Al results. Greater distribution of CoQtz-N targets from individual laboratories to several AMS facilities would help address these issues and such tests will be implemented in the near future.

5. Conclusions

Initial ^{10}Be and ^{26}Al results of CoQtz-N show that it is suitable as an in-house reference material and for inter-laboratory comparisons. Based on the available results, consensus values for ^{10}Be and ^{26}Al in CoQtz-N are $2.54\text{--}53 \pm 0.02\text{--}09 \times 10^6$ at/g and $15.6 \pm 1.6\text{--}15.7 \pm 0.4 \times 10^6$ at/g, respectively, at the [estimated](#) 95% confidence limit. These values should be considered preliminary and the ^{26}Al value in particular is likely to be subject to changes in the future as more results are forthcoming. ~~Though there are statistically significant differences in ^{10}Be concentrations between some laboratories, it~~ is encouraging that ~~there appears a the majority show~~ reasonable agreement [in \$^{10}\text{Be}\$ concentrations prepared in different laboratories and measured on several AMS](#). ^{26}Al concentration measurements show less concordance and clearly require focused attention in future. It is not yet clear whether the differences we observe stem from the target preparation or the AMS measurement. More measurements from a single laboratory at multiple AMS facilities would help address this and ongoing determinations will help to improve our understanding of what is causing dispersion. To obtain a split of CoQtz-N contact S. Binnie or T. Dunai.

Acknowledgements

We thank Tomasz Goral at the University of Cologne, Elaine McDougall at the University of Edinburgh and Irene Schimmelpfennig at CEREGE for helping facilitate this research. [We thank an anonymous reviewer and Lee Corbett for comments that helped improve the quality of our manuscript. We are also very grateful to Marian Scott for introducing us to mixed modelling.](#)

References

- Bevington P. R., D.K. Robinson D.K., (2003) Data Reduction and Error Analysis for the Physical Sciences (3rd ed), (McGraw Hill, New York) pp. 320.
- Bierman P., T. Brown, M. Caffee, L. Corbett, D. Fink, S. Freeman, A.J. Hidy, D. Rood, K. Wilcken, T. Woodruff, S. Zimmerman, (2017) Repeated preparation of CRONUS-N quartz standard for ¹⁰Be and ²⁶Al at the University of Vermont and analysis at four different AMS laboratories, The 14th International Conference on Accelerator Mass Spectrometry, August 14th-18th Ottawa, Canada.
- Binnie, S.A., T.J. Dunai, E. Voronina, T. Goral, S. Heinze, A. Dewald, Separation of Be and Al for AMS using single-step column chromatography, Nuclear Instruments & Methods in Physics Research Section B-Beam Interactions with Materials and Atoms, 361 (2015) 397-401.
- Blard, P.H., G. Balco, P.G. Burnard, K.A. Farley, C.R. Fenton, R. Friedrich, A.J.T. Jull, S. Niedermann, R. Pik, J.M. Schaefer, E.M. Scott, D.L. Shuster, F.M. Stuart, M. Stute, B. Tibari, G. Winckler, L. Zimmermann, An inter-laboratory comparison of cosmogenic He-3 and radiogenic He-4 in the CRONUS-P pyroxene standard, Quaternary Geochronology, 26 (2015) 11-19.
- Child, D., G. Elliott, C. Mifsud, A.M. Smith, D. Fink, Sample processing for earth science studies at ANTARES, Nuclear Instruments & Methods in Physics Research Section B-Beam Interactions with Materials and Atoms, 172 (2000) 856-860.
- Corbett, L.B., P.R. Bierman, D.H. Rood, An approach for optimizing in situ cosmogenic Be-10 sample preparation, Quaternary Geochronology, 33 (2016) 24-34.
- Dean, R.B., W.J. Dixon, Simplified Statistics for Small Numbers of Observations, Anal Chem, 23 (1951) 636-638.

Fujioka, T., D. Fink, C. Mifsud, Towards improvement of aluminium assay in quartz for in situ cosmogenic Al-26 analysis at ANSTO, Nuclear Instruments & Methods in Physics Research Section B-Beam Interactions with Materials and Atoms, 361 (2015) 346-353.

Granger, D.E., N.A. Lifton, J.K. Willenbring, A cosmic trip: 25 years of cosmogenic nuclides in geology, Geological Society of America Bulletin, 125 (2013) 1379-1402.

Hunt, A.L., J. Larsen, P.R. Bierman, G.A. Petrucci, Investigation of factors that affect the sensitivity of accelerator mass spectrometry for cosmogenic Be-10 and Al-26 isotope analysis, Anal Chem, 80 (2008) 1656-1663.

Hunt, A.L., G.A. Petrucci, P.R. Bierman, R.C. Finkel, Metal matrices to optimize ion beam currents for accelerator mass spectrometry, Nuclear Instruments & Methods in Physics Research Section B-Beam Interactions with Materials and Atoms, 243 (2006) 216-222.

Jull, A.J.T., E.M. Scott, P. Bierman, The CRONUS-Earth inter-comparison for cosmogenic isotope analysis, Quaternary Geochronology, 26 (2015) 3-10.

Kohl, C.P., K. Nishiizumi, Chemical isolation of quartz for measurement of in situ-produced cosmogenic nuclides, Geochimica Et Cosmochimica Acta, 56 (1992) 3583-3587.

Ku., H.H., Statistical Concepts in Metrology, in Precision Measurement and Calibration: Statistical Concepts and Procedures, Ku, H.H. (ed), National Bureau of Standards Special Publication 300, (1969) Vol. 1. (National Bureau of Standards, Gaithersburg).

Merchel, S., and W. Bremser, First international ²⁶Al interlaboratory comparison – Part I, Nuclear Instruments & Methods in Physics Research Section B-Beam Interactions with Materials and Atoms, 223-224 (2004) 393-400

Merchel, S., M. Arnold, G. Aumaitre, L. Benedetti, D.L. Bourles, R. Braucher, V. Alfimov, S.P.H.T. Freeman, P. Steier, A. Wallner, Towards more precise (10)Be and (36)Cl data from measurements at the 10(-14) level: Influence of sample preparation, Nuclear Instruments & Methods in Physics Research Section B-Beam Interactions with Materials and Atoms, 266 (2008) 4921-4926.

Merchel, S., W. Bremser, S. Akhmaliev, M. Arnold, G. Aumaitre, D.L. Bourles, R. Braucher, M. Caffee, M. Christl, L.K. Fifield, R.C. Finkel, S.P.H.T. Freeman, A. Ruiz-Gomez, P.W. Kubik, M. Martschini, D.H. Rood, S.G. Tims, A. Wallner, K.M. Wilcken, S. Xu, Quality assurance in accelerator mass spectrometry: Results from an international round-robin exercise for Be-10, Nuclear Instruments & Methods in Physics Research Section B-Beam Interactions with Materials and Atoms, 289 (2012) 68-73.

Merchel, S., W. Bremser, D.L. Bourles, U. Czeslik, J. Erzinger, N.A. Kummer, L. Leanni, B. Merkel, S. Recknagel, U. Schaefer, Accuracy of Be-9-data and its influence on Be-10 cosmogenic nuclide data, J Radioanal Nucl Ch, 298 (2013) 1871-1878.

Mifsud, C., T. Fujioka, D. Fink, Extraction and purification of quartz in rock using hot phosphoric acid for in situ cosmogenic exposure dating, Nuclear Instruments & Methods in Physics Research Section B-Beam Interactions with Materials and Atoms, 294 (2013) 203-207.

Nishiizumi, K., Preparation of Al-26 AMS standards, Nuclear Instruments & Methods in Physics Research Section B-Beam Interactions with Materials and Atoms, 223 (2004) 388-392.

Nishiizumi, K., M. Imamura, M.W. Caffee, J.R. Southon, R.C. Finkel, J. McAninch, Absolute calibration of Be-10 AMS standards, Nuclear Instruments & Methods in Physics Research Section B-Beam Interactions with Materials and Atoms, 258 (2007) 403-413.

Phillips, F.M., D.C. Argento, G. Balco, M.W. Caffee, J. Clem, T.J. Dunai, R. Finkel, B. Goehring, J.C. Gosse, A.M. Hudson, A.J.T. Jull, M.A. Kelly, M. Kurz, D. Lal, N. Lifton, S.M. Marrero, K. Nishiizumi, R.C. Reedy, J. Schaefer, J.O.H. Stone, T. Swanson, M.G. Zreda, The CRONUS-Earth Project: A synthesis, Quaternary Geochronology, 31 (2016) 119-154.

Rozanski, K., W. Stichler, R. Gonfiantini, E.M. Scott, R.P. Beukens, B. Kromer, J. Vanderpligt, The IAEA C-14 Intercomparison Exercise 1990, Radiocarbon, 34 (1992) 506-519.

Scott, E.M., The Third International Radiocarbon Intercomparison (TIRI) and the Fourth International Radiocarbon (FIR) - 1999-2002 - Results, analysis and conclusions, Radiocarbon, 45 (2003) Vii-X.

Scott, E.M., G.T. Cook, P. Naysmith, Error and uncertainty in radiocarbon measurements, Radiocarbon, 49 (2007) 427-440.

[Scott, E.M., P. Naysmith and G.T. Cook, Should archaeologists care about 14C inter-comparisons? Why? A summary report on SIIRI, Radiocarbon, 59\(5\) \(2017\) 1589-1596.](#)

Stone, J., K. Fifield, J. Beer, M. Vonmoos, C. Obrist, M. Grajcar, P. Kubik, R. Muscheler, R. Finkel, M. Caffee, Co-precipitated silver-metal oxide aggregates for accelerator mass spectrometry of Be-10 and Al-26, Nuclear Instruments & Methods in Physics Research Section B-Beam Interactions with Materials and Atoms, 223 (2004) 272-277.

Taylor, J.K., (1987) Quality Assurance of Chemical Measurements, pp328, (Lewis Publishers, Michigan)

Vermeesch, P., G. Balco, P.H. Blard, T.J. Dunai, F. Kober, S. Niedermann, D.L. Shuster, S. Strasky, F.M. Stuart, R. Wieler, L. Zimmermann, Interlaboratory comparison of cosmogenic Ne-21 in quartz, Quaternary Geochronology, 26 (2015) 20-28.

Ward, G.K., S.R. Wilson, Procedures for Comparing and Combining Radiocarbon Age-Determinations - Critique, Archaeometry, 20 (1978) 19-31.

Wendt, I., C. Carl, The Statistical Distribution of the Mean Squared Weighted Deviation, Chemical Geology, 86 (1991) 275-285.

Figure captions

Figure 1. The starting material for CoQtz-N was the single boulder of vein quartz indicated.

Figure 2. ^{10}Be measurements of CoQtz-N that have undergone further HF/HNO₃ etching in addition to that undertaken during bulk preparation. The ^{10}Be concentrations are unaffected by more etches, suggesting the material is free of any adsorbed meteoric ^{10}Be .

Figure 3a. ^{10}Be measurements of CoQtz-N from AMS 1 display a positive relationship with the analytical ^9Be current of the individual targets, represented as a fraction of the average current of the standards in the same run (relative ^9Be current). A linear relationship is indicated ($r = 0.43$) and the grey lines are the 95% confidence intervals. **3b** shows the ^{10}Be concentrations of the same samples as in figure 3a following normalization to the average standard currents from the same run.

Figure 4. CoQtz-N ^{10}Be measurements from each laboratory where the targets were prepared. Each laboratory is given a different colored symbol and labelled as Lab 1 through Lab 11. The shape of the symbols refers to the accelerator mass spectrometers where the targets were measured, labelled AMS 1 through AMS 7. Error bars are one standard deviation, the thick grey line is the arithmetic mean of all measurements and the thinner grey lines are the 95% confidence intervals of the mean. The asterisk (*) denotes a potential outlier from laboratory 1 (see main text for more details).

Figure 5. CoQtz-N ^{26}Al measurements from each laboratory where the targets were prepared. Colors and symbols are the same as used in Figure 4. Error bars are one standard deviation, the thick grey line is the arithmetic mean of all measurements and the thinner grey lines are the 95% confidence intervals of the mean.

Formatted: Highlight

Figure 6. The upper plot shows all ^{10}Be concentrations with the same symbol color and shape scheme as in Figure 4. The lower plot shows the corresponding reagent blank subtractions for each individual measurement.

Figure 7a. Arithmetic mean ^{10}Be values for each target preparation laboratory where two or more results were obtained and the corresponding 95% confidence intervals where there are 3 or more results (see Table 3). The median ^{10}Be concentration, indicated by the red squares, is also derived for laboratories with three or more results. **7b.** as in **7a** but for ^{26}Al results. See Table 4 for details.

Figure 8. Ranked ^{10}Be concentrations measurements of CoQtz-N, including one standard deviation uncertainties on the individual measurement. The 13 red circles are the measurements that are rejected prior to the derivation of the error weighted mean, according to Rozanski et al. (1992). The error weighted mean ^{10}Be concentration is given by the black line and the estimated 95% confidence intervals of the weighted mean are illustrated by the green lines. Note the confidence intervals are derived from the estimated standard error of the weighted mean.

Figure 9. Ranked ^{26}Al concentrations measurements of CoQtz-N including one standard deviation uncertainties on the individual measurements. The four red circles are the measurements that are rejected prior to the derivation of the error weighted mean, according to Rozanski et al. (1992). The error weighted mean ^{26}Al concentration is given by the ~~blank-black~~ line and the estimated 95% confidence intervals of the weighted mean are illustrated by the green lines. Note the confidence intervals are derived from the estimated standard error of the weighted mean.

Figure 1 (single column width). Online version (greyscale copy to be provided for print version).

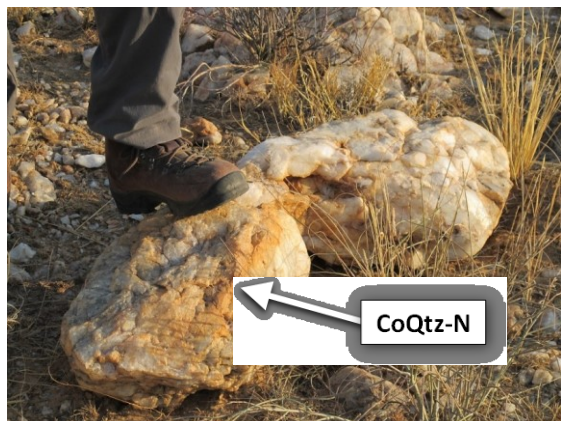


Figure 2 (single column width).

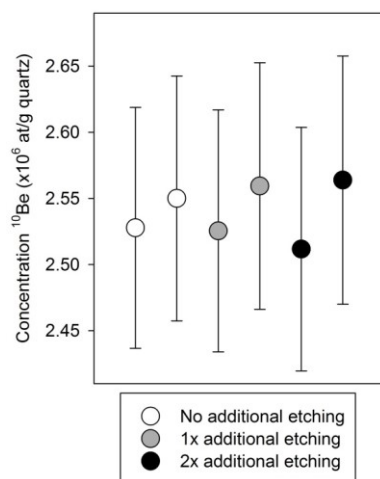


Figure 3 (single column width). Online version (greyscale copy to be provided for print version).

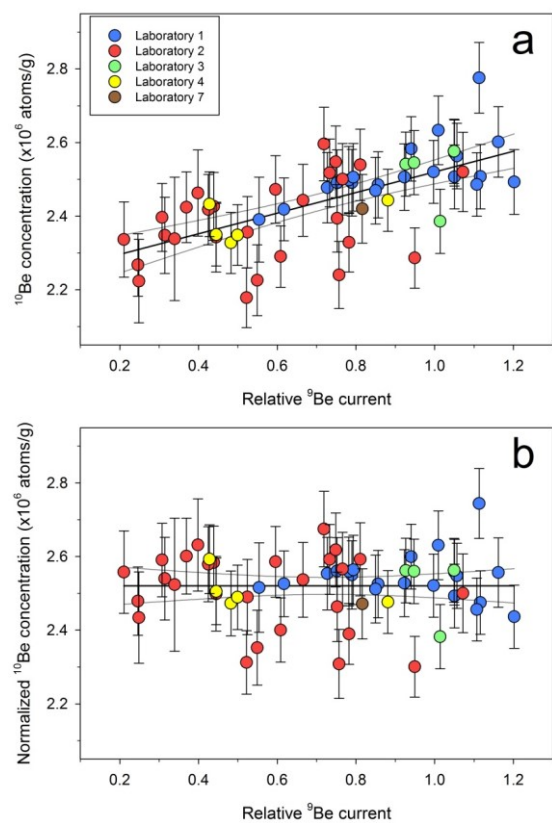


Figure 4 (double column width). Online version (greyscale copy to be provided for print version).

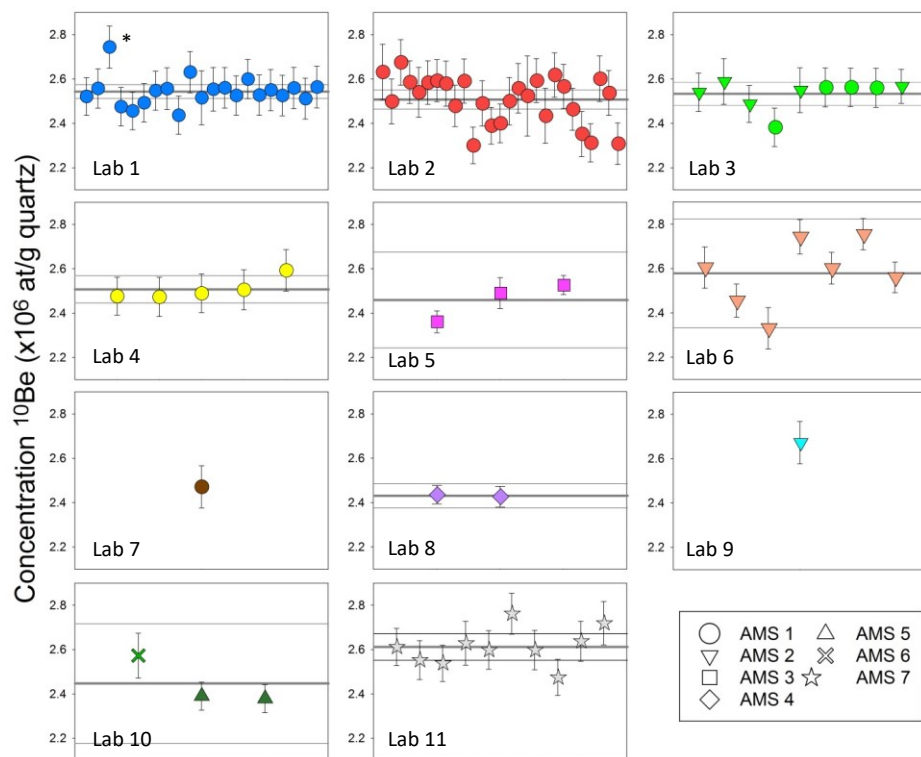


Figure 5 (single column width). Online version (greyscale copy to be provided for print version).

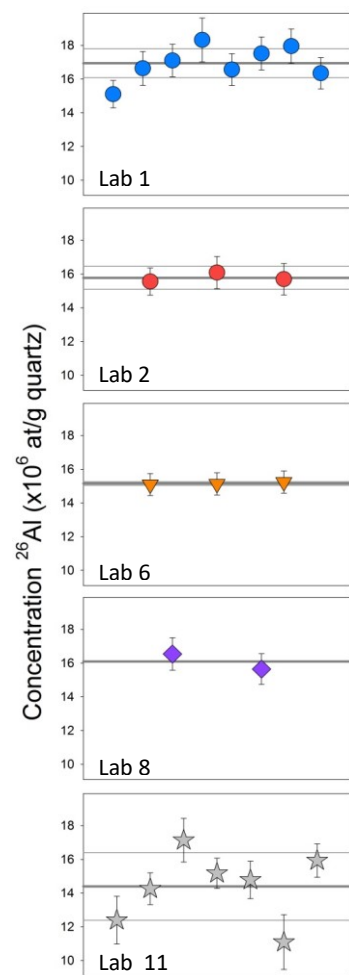


Figure 6 (double column width). Online version (greyscale copy to be provided for print version).

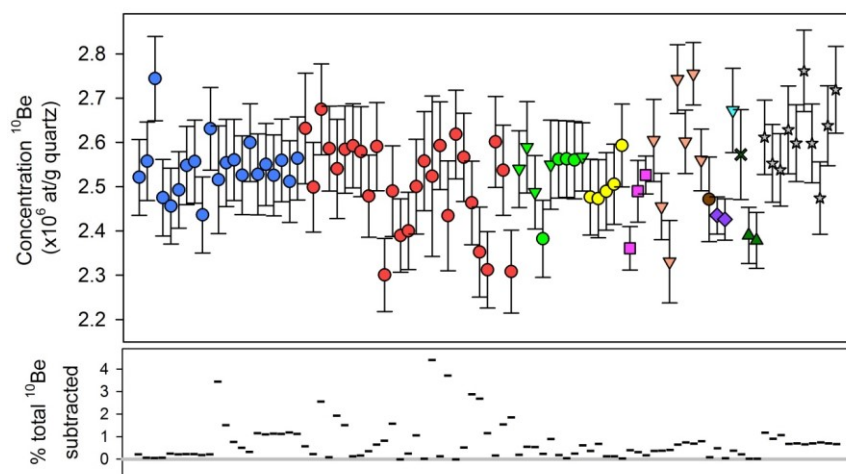


Figure 7 (single column width). Online version (greyscale copy to be provided for print version).

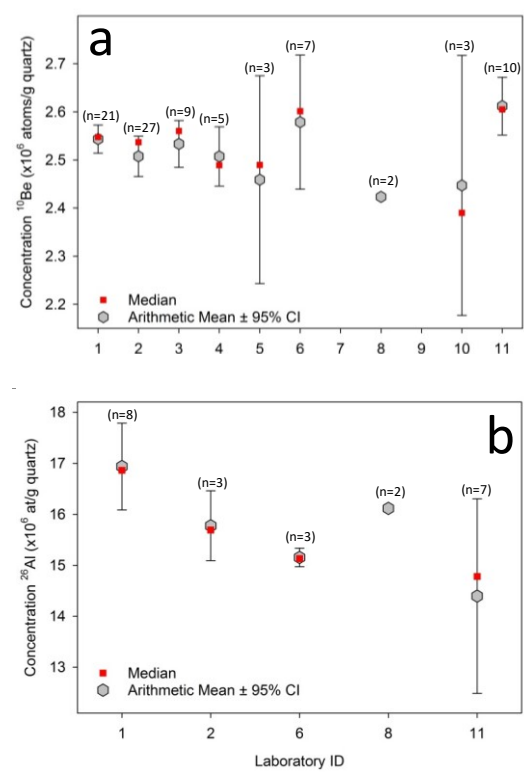


Figure 8 (single column width). Online version (greyscale copy to be provided for print version).

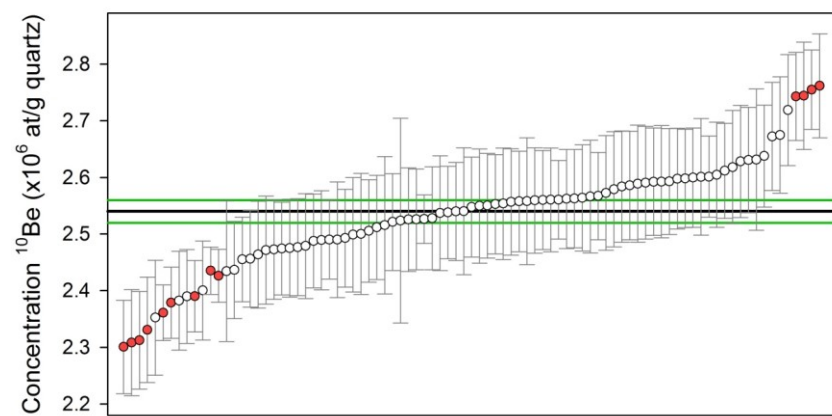


Figure 9 (single column width). Online version (greyscale copy to be provided for print version).

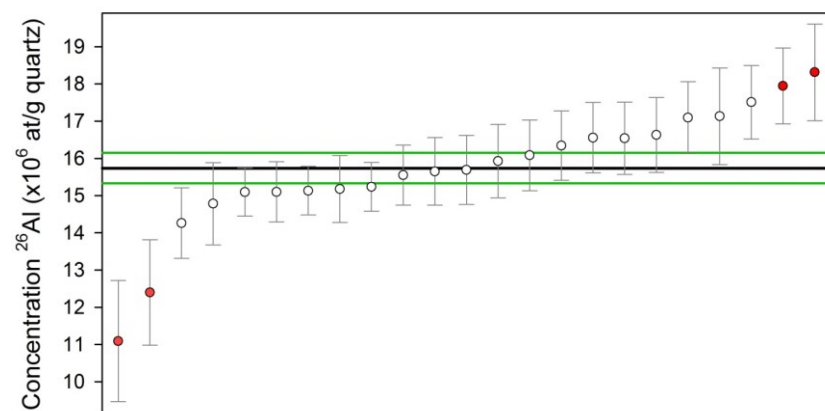


Table 1. (Single column width)

Table 1.
Participating laboratories and AMS
facilities (alphabetical order)

<p><u>Target Preparation Laboratories</u></p> <ul style="list-style-type: none"> • Australian Nuclear Science and Technology Organisation (ANSTO) • Centre Européen de Recherche et d'Enseignement des Géosciences de l'Environnement (CEREGE) • Eidgenössische Technische Hochschule (ETH-Zurich) • GeoForschungsZentrum (GFZ) • Scottish Universities Environmental Research Centre (SUERC) • University of Bremen • University of Bern • University of Cologne • University of Münster • University of Tübingen • University of Wollongong <p><u>Participating AMS Facilities</u></p> <ul style="list-style-type: none"> • Accélérateur pour les Sciences de la Terre, Environnement, Risques (ASTER) • Australian National University (ANU) • Australian Nuclear Science and Technology Organisation (ANSTO)* • Eidgenössische Technische Hochschule (ETH-Zurich) • Scottish Universities Environmental Research Centre (SUERC) • University of Cologne (CologneAMS)

*Measurements made on two AMS, Antares and Sirius.

Table 2 (Single column width)

Table 2: CoQtz-N major elements by ICP-OES

Element	CoQtz-N concentration ¹
Na	7.7 ± 1.9
Al	18.4 ± 0.6
K	2.3 ± 1.6
Ca	1.3 ± 0.1
Ti	7.6 ± 2.6
Fe	16.6 ± 14.5

All of Be, B, Mg and Mn are sub-ppm

¹ Mean and 1 standard deviation (n=5).
 Measured in-house at University of Cologne
 on a Spectro Arcos ICP-OES, using standard
 addition (four dilutions), wavelengths (nm):
 Be 313.107; B 249.773; Na 589.592; Mg
 280.270; Al 167.078; K 766.491; Ca 396.847;
 Ti 334.941; Mn 257.611; Fe 261.187.

Table 3 (Double column width)

Table 3.

Different measures of ^{10}Be concentration central tendency. s.d. and s.e. refer to the standard deviation and standard error, respectively. HL and HU refer to the lower and upper quartiles (hinges). The mean square weighted deviation (MSWD) is included for laboratories that have reported seven or more measurements.

Target Prep. Lab.	AMS fac.	N	Arithmetic Mean	± 1 s.d.	± 1 s.e.	95% Confidence Interval [LL - UL]	Error Weighted Mean (EWM)	Estimated ± 1 s.e. of the EWM	Median	Quartiles [H _L - H _U]	MSWD
(x10 ⁶ at/g quartz)											
1	1	21	2.54	0.06	0.01	2.51 - 2.57	2.54	0.02	2.55	2.52 - 2.56	0.49
2	1	27	2.51	0.11	0.02	2.47 - 2.55	2.50	0.02	2.54	2.45 - 2.59	1.27
3 [§]	1,2	9	2.53	0.06	0.02	2.48 - 2.58	2.53	0.03	2.56	2.54 - 2.56	0.52
4	1	5	2.51	0.05	0.02	2.45 - 2.57	2.50	0.04	2.49	2.48 - 2.51	.
5	3	3	2.46	0.09	0.05	2.24 - 2.67	2.46	0.03	2.49	.	.
6	2	7	2.58	0.15	0.06	2.44 - 2.72	2.59	0.03	2.60	2.51 - 2.67	3.46
7*	1	1	2.47	0.10
8	4	2	2.43	0.00	0.00	.	2.43	0.03	.	.	.
9*	2	1	2.67	0.10
10 [§]	5,6	3	2.45	0.11	0.06	2.18 - 2.72	2.41	0.04	2.39	.	.
11	Z	10	2.61	0.08	0.03	2.55 - 2.67	2.60	0.03	2.60	2.56 - 2.64	0.90

* A single measurement is reported by these laboratories, the single value and quoted uncertainty are shown under arithmetic mean and standard deviation.

§ Where two AMS facilities have been used the statistics are derived using the combined measurements from both.

Formatted Table

Formatted: Superscript

Formatted: Superscript

Table 4 (Double column width)

Table 4.

Different measures of ^{26}Al concentration central tendency. s.d. and s.e. refer to the standard deviation and standard error, respectively. HL and HU refer to the lower and upper quartiles (hinges). The mean square weighted deviation (MSWD) is included for laboratories that have reported seven or more measurements.

Formatted Table

Target Prep. Lab.	AMS FaC.	n	Arithmetic Mean	± 1 s.d.	± 1 s.e.	95% Confidence Interval [LL - UL]	Error Weighted Mean (EWM)	Estimated ± 1 s.e. of the EWM	Median	Quartiles [HL - HU]	MSWD
(x10 ⁶ at/g quartz)											
1	1	8	16.9	1.0	0.4	16.1 – 17.8	16.7	0.3	16.9	16.5 - 17.6	1.18
2	1	3	15.8	0.3	0.2	15.1 – 16.5	15.7	0.5	15.7	.	.
6	2	3	15.2	0.1	0.0	15.0 – 15.3	15.2	0.4	15.1	.	.
8	4	2	16.1	0.6	0.4	.	16.1	0.7	.	.	.
11	7	7	14.4	2.1	0.8	12.5 – 16.3	14.8	0.4	14.8	13.3 - 15.6	2.32

Table 5 (Single column width)

Table 5.

Results of an ANOVA test of ^{10}Be concentrations of laboratories 1, 2, 2 and 11. F is the ratio of the mean squares of between groups and within groups and determines the significance level (P value) for the specified degrees of freedom. When F is large it indicates that the inter-laboratory scatter is more than would be expected to occur by chance when compared with the intra-laboratory scatter. The average values and confidence intervals for concentrations of ^{10}Be and ^{26}Al in CoQtz-N derived using the three different approaches described in detail in the main text.

Averaging approach used	Average ^{10}Be concentration \pm 95% Confidence Interval ($\times 10^6$ at ^{10}Be /g)	Average ^{26}Al concentration \pm 95% Confidence Interval ($\times 10^6$ at ^{26}Al /g) Mean Squares
Between-groups Grand Average	2.53 ± 0.028 0.049E+10	15.2 ± 0.12 683E+10
Within-groups Filtered EWM	2.54 ± 0.024 665E+11	15.7 ± 0.47 406E+09
Total Linear Mixed Modeling	2.53 ± 0.09 5.470E+11	15.6 ± 1.6

Formatted Table

Formatted: Superscript

Formatted: Superscript

Formatted: Superscript

Formatted: Superscript